



(51) International Patent Classification:

A61F 2/28 (2006.01) B29C 33/62 (2006.01)
A61F 2/30 (2006.01) B29C 33/68 (2006.01)

(21) International Application Number:

PCT/EP2016/071927

(22) International Filing Date:

16 September 2016 (16.09.2016)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

15185395.9 16 September 2015 (16.09.2015) EP

(71) Applicants: **3D-SIDE** [BE/BE]; Fond des Més 4, 1348 Ottignies-Louvain-la-Neuve (BE). **UNIVERSITÉ CATHOLIQUE DE LOUVAIN** [BE/BE]; Place de l'Université 1, 1348 Louvain la Neuve (BE).

(72) Inventors: **HEUNEN, Guido**; Place des Peintres 1, 104, 1348 Louvain la Neuve (BE). **SCLAVONS, Michel**; 81, avenue Jean-François Debecker, 1200 Woluwe-Saint-Lambert (BE). **KINET, Christine**; Avenue Echevin Van Muylders 12, 1200 Woluwe-Saint-Lambert (BE). **TRAN DUY, Khanh**; Rue du Maieur 29, 1457 Walhain (BE). **PAUL, Laurent**; Rue Adjudant Kumps, 75, 1495 Mellery (BE).

(74) Agent: **ICOSA**; 83 avenue Denfert-Rochereau, 75014 Paris (FR).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Declarations under Rule 4.17:

— of inventorship (Rule 4.17(iv))

[Continued on next page]

(54) Title: IMPLANT MOLDING SYSTEM

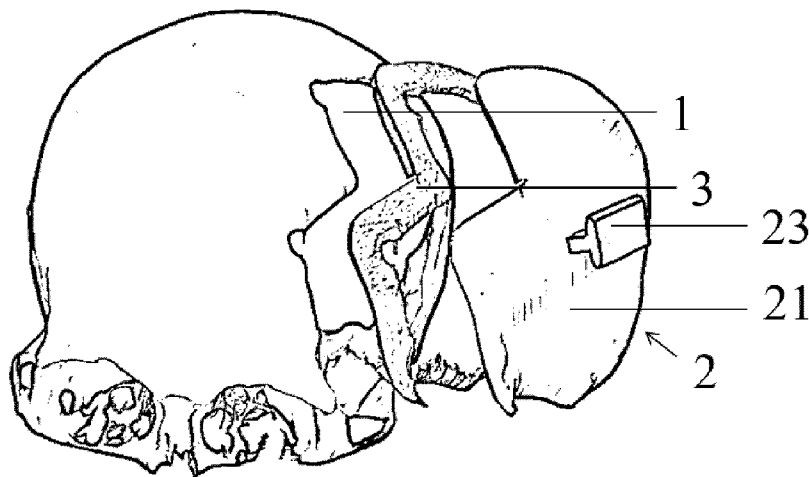


FIG. 3

(57) Abstract: The present invention relates to an implant molding system for the molding of an hardenable implant forming material comprising a mold (2) obtainable from an image of a bone defect (1) by additive manufacturing and having a surface concave along at least one axis; and tangible means for retaining the implant forming material in the mold during hardening and for unmolding the implant thereafter; wherein said tangible means for retaining the implant forming material in the mold during hardening and for unmolding after hardening comprises or consists of a coating to be applied onto the concave surface of the mold.

Published:

— *with international search report (Art. 21(3))*

IMPLANT MOLDING SYSTEM

FIELD OF INVENTION

The present invention relates to the field of molding systems for the manufacture of
5 implants such as for example cranial implants. In particular, the present invention relates
to an implant molding system for the molding of a hardenable implant forming material
comprising both a mold and means for retaining the implant forming material in the mold
during hardening and for unmolding the hardened implant.

10 BACKGROUND OF INVENTION

In numerous situations, it may be necessary to repair cranial defects by means of cranial
implants. These defects can arise from traumas, craniectomies, tumors or malformations.
Cranioplasty is a neurosurgical procedure enabling to restore the protection of the brain
and to improve esthetic appearance. However, the accurate restoration of the missing part
15 is particularly challenging.

Three materials are currently available to repair bone defects: autografts, allografts and
biomaterials. Autografts and allografts are naturally limited (autograft) or raises
biocompatibility issues (allograft). Biomaterials may be used during surgery to
manufacture implants in situ: for instance some surgeons use a glove to directly shape the
20 bone cement onto a cranial defect. However, said method is known as being time-
consuming and depends on the ability of the surgeon.

The development of computer assisted design and rapid prototyping technology increases
significantly the possibility to preoperatively manufacture precise and adapted implants
from biomaterials and cranial scan data. However, the scan data may not be fully reliable
25 due to patient movement during the imaging or could become irrelevant if the surgeon
decides to enlarge the bone defect during the surgery (e.g. in the case of the spread of a
bone tumor). Therefore preoperatively-made implants from cranial scan data could be
inappropriate to restore full protection of the brain. In order to ensure protection of the

brain, optimal stress distribution along the periphery of the implant as well as the esthetic appearance; the curvature of the skull of each patient must be respected. The outer surface of the implant should be flush with the outer surface of the skull along the periphery of the implant. According to the applicant, meeting said feature with a preoperatively-made
5 implant is one of the issue faced at each surgery.

It is thus an aspect of the present invention to provide an implant molding system for the manufacture of an implant restoring the protection of the brain while ensuring a continuous outer curvature at the boundary between the skull of the patient and the implant.

10 To that end, the implant molding system for the molding of an hardenable implant forming material comprises:

- a mold comprising a bottom plate; and
- means for retaining the implant forming material in the mold during hardening and for unmolding the implant after hardening.

15 The means for retaining the implant forming material in the mold during hardening and for unmolding the implant after hardening ensure unmolding of the implant while also avoiding contamination of the implant forming material by the material of the mold. As the mold ensures the correct curvature of the outer surface of the implant, due to the bottom plate, without limiting the lateral sizes of the implant, said mold may be generated
20 using imaging such as cranial scan data of a patient having a bone defect; thereby avoiding the drawbacks of the prior art.

SUMMARY

The present invention relates to an implant molding system for the molding of an
25 hardenable implant forming material comprising: a mold obtainable from an image of a bone defect by additive manufacturing and having a surface concave along at least one axis; and tangible means for retaining the implant forming material, for instance against gravity, in the mold during hardening and for unmolding the implant after hardening; wherein said tangible means for retaining the implant forming material in the mold during

hardening and for unmolding after hardening comprises or consists of a coating to be applied onto the concave surface of the mold wherein said coating is made of a biocompatible material and said coating has a phase transition temperature ranging from 40 to 100°C.

- 5 According to one embodiment, the coating is selected from homopolymer or copolymer of poly(isoprene), poly(chloroprene), poly(vinyl alcohol), poly(acrylonitrile), poly(butadiene), poly(vinyl chloride), poly(ethylene), poly(isobutylene), poly(ethylene glycol), poly(lactic acid) or any mixtures thereof.

- According to one embodiment, the coating is selected from vaseline or wax or any mixtures thereof. According to one embodiment, the coating is vaseline. According to
10 one embodiment, the coating is Horsley's wax.

- According to one embodiment, the coating is selected from homopolymer or copolymer of poly(isoprene), poly(chloroprene), poly(vinyl alcohol), poly(acrylonitrile), poly(butadiene), poly(vinyl chloride), poly(ethylene), poly(isobutylene), poly(ethylene
15 glycol), poly(lactic acid); or vaseline or wax or any mixtures thereof.

According to one embodiment, the coating forms a solid layer at a temperature ranging from 0 to 40°C, preferably from 25 to 40°C.

- According to one embodiment, the coating is applied onto the concave surface of the mold in solid form. According to one embodiment, the coating further comprises a tab
20 extending outside of the mold enabling peeling said coating off the mold. According to one embodiment, the coating is selected from poly(acrylonitrile-co-butadiene).

- According to another embodiment, the coating is applied onto the concave surface of the mold in liquid form. According to one embodiment, the coating exhibits a melting temperature above T1 and below T2, wherein T1 is ranging from 0 to 40°C, preferably
25 from 25 to 40°C and wherein T2 is ranging from ranging from 45 to 100°C, preferably from 70 to 90°C. According to one embodiment, the coating is selected from homopolymer or copolymer of poly(ethylene glycol). According to one embodiment, the coating is selected from a crystalline, semicrystalline or amorphous material; preferably,

the coating is selected from material having a glass temperature lower than the reaction temperature.

According to one embodiment, the implant molding system according to the invention further comprises a molding ring having a negative surface profile relative to the mold,
5 an inner edge and a predefined thickness along the edge.

According to one embodiment, the implant molding system further comprises a forming tool having a negative surface profile relative to the mold, such that joining the forming tool with the mold, and optionally with the molding ring, forms a cavity.

According to one embodiment, the implant molding system further comprises a counter
10 mold comprising a first and a second counter mold portion, each comprising an inner part and an outer part, wherein the counter mold and the mold form, when mated together, a cavity corresponding to the image of the bone defect.

According to one embodiment, the surface concave along at least one axis conforms to an arc with a radius ranging from 2 to 20 centimeters, from 4.5 to 9.5 centimeters, or
15 substantially equal to 7 centimeters.

According to one embodiment, the mold and/or the molding ring and/or the forming tool and/or the counter mold comprises a material selected from ceramics, metals, metal alloys, glasses, polymers, bone or portland like cement, gypsum, sand or a mixture thereof.

20 According to one embodiment, the implant molding system according to the invention further comprises an implant forming composition comprising a liquid phase comprising at least one liquid monomer, and at least one polymerization inhibitor; and a solid phase comprising at least one polymer, at least one initiator; optionally at least one activator, and optionally at least one radio-opaque filler.

DEFINITIONS

In the present invention, the following terms have the following meanings:

- **“Additive manufacturing”** refers to a manufacturing process for shaping objects by successive addition of material.
- 5 - **“Bone defect”** refers to a part of a bone of a subject that will not heal without intervention or to the part of a bone removed during a surgery having a size ranging from 5 to 400 cm², preferably from 30 to 150 cm².
- **“Coating”** refers to a covering that is applied on a surface and forms a layer of solid or viscous material.
- 10 - **“Harden”** or **“hardening”** refers to the action to make or to become hard or harder. According to the present invention, said action may be implemented by chemical or physical means; preferably by chemical means. According to the present invention, “harden” or “hardening” also includes when said action is implemented by using a cross-linking agent (“curing”).
- 15 - **“Implant forming material”** refers to any material that may be formed by molding to generate a surgical prosthesis for a defect, preferably said material is hardenable.
- **“Mold”** refers to a curved plate having at least one predefined curvature either concave or convex, preferably predefined by the specific curvature of the outer surface of the bone of a patient with a bone defect.
- 20 - **“Monomer”** refers to compound bearing at least one function allowing the polymerization of said compound by a radical or a condensation reaction.
- **“Phase transition temperature”** refers to the temperature needed for the material to pass from a solid or viscous phase to a liquid phase.
- **“Reaction temperature”** refers to the highest temperature reached during hardening
25 of the implant forming material.
- **“Subject”** or **“patient”** refers to an animal, preferably a mammal, more preferably a human, in need of an implant.

- “**Substantially**” and “**about**” refer, when used in conjunction with a numerical value, to the variation above or below 10% of said value, preferably above or below 5% of said value.
- “**Viscosity**” refers to the uniform flow resistance (without turbulence) occurring in the mass of a material. In the case of a polymer solution, said viscosity depends on the temperature and the concentration of said polymer solution and its molecular weight and structure.
- “**Viscous**” refers herein to a compound having a viscosity value higher than 80mPa.s at 20°C. The viscosity may be measured by any appropriate viscometer, method or apparatus known by the skilled artisan, such as but not limited to, viscometer of Oswald or Ubbelohde, falling ball viscometer, rotative or Couette viscometer.

DETAILED DESCRIPTION

This invention relates to an implant molding system for the molding of an hardenable implant forming material comprising:

- a mold **2** having at least one predefined curvature;
- means for retaining the implant forming material in the mold **2** during hardening and for unloading the hardened implant, especially tangible means; and
- optionally a molding ring **3**.

According to one embodiment, the implant molding system is used for manufacturing implants in human and veterinary medicine. According to a preferred embodiment, the implant molding system is used for manufacturing implants such as cranial implants, preferably neurocranial implant. According to a preferred embodiment, the implant molding system is used for manufacturing implants to repair bone defect as shown in figure 1. However, the present invention is not limited to cranial implant and one skilled in the art could use the implant molding system of the invention to manufacture other implants such as for instance zygomatic implants, maxillofacial implants, chin implants or pelvic implants.

According to a first embodiment, the mold **2** comprises a surface concave along at least one axis. According to one embodiment, the mold **2** comprises a partly concave surface along at least one axis. According to another embodiment, the mold **2** comprises a surface convex along at least one axis. According to one embodiment, the mold **2** comprises a partly convex surface along at least one axis. According to one embodiment, the surface of the mold **2** is concave and substantially conforms to an arc with a radius ranging from 2 to 20 centimeters, preferably from 4.5 to 9.5 centimeters, or substantially equal to 7 centimeters.

According to one embodiment, the mold **2** comprises an inner face **22** and an outer face **21** as shown in figure 2A and 2B. The said inner face **22** is designed to be in contact with the implant forming material and the said outer face **21** is oriented towards outward. According to one embodiment, the mold **2** comprises a handle **23** on its outer face **21**.

According to one embodiment, the mold **2** has the shape of the bone defect **1** to be replaced or restored. According to one embodiment, the mold **2** is patient-specific. According to one embodiment, the mold **2**, which has the shape of the bone defect **1** to be replaced or restored, is designed via medical imaging. It may be manufactured by additive manufacturing such as 3D printing.

According to one embodiment, a digital imaging system, such as for example a computer tomography (CT) or Magnetic resonance imaging (MRI) is used to obtain an imaging data pertaining to a patient's anatomy. The imaging data is then imported into a standard image format by use of a suitable software, such as for example Mimics® (Materialise). This enables the creation of a 3D model of the patient anatomy. Having obtained a 3D model of the patient anatomy, a model of the mold **2** having a surface corresponding to the bone defect **1** including size and curvature thereof is produced. From the model, the mold **2** is processed and manufactured by any technique known by one skilled in the art such as additive manufacturing (e.g. binder jetting, material extrusion, material jetting, powder bed fusion, sheet lamination, selective laser sintering, sheet metal forming...). Thus according to one embodiment, the mold **2** has a curvature ensuring continuity and/or tangency at the boundary between the bone of the patient, for instance a skull, and the

implant. According to one embodiment, the mold **2** has a curvature ensuring flush with the boundary between the bone of the patient, for instance a skull, and the implant.

According to one embodiment, the mold is obtained by adapting a standard plate or a standard mold to a desired implant shape, for instance by bending and/or forming.

5 According to an alternative embodiment, the mold **2** is generated from bone models having standard curvatures. For instance, the mold **2** is generated from a skull model having standard curvature. The curvature of the skull typically ranges from 2 centimeters to 20 centimeters, preferably from 4.5 to 9.5 centimeters or is approximately equal to 7 centimeters. The standard mold may then be adapted during surgery to the patient
10 anatomy to be perfectly flush.

According to one embodiment, the mold **2** is manufactured preoperatively. According to one embodiment, the mold **2** is manufactured per-operatively.

According to one embodiment, the mold **2** has a surface larger than the size of the bone defect to be repaired or restored. Preferably, the mold **2** has a surface larger than the size
15 of the bone defect to be replaced such that the surgeon may use the mold **2** even if he decides during the surgery to enlarge the bone defect for medical reason. According to one embodiment, the edge of the mold **2** corresponds to the edge of the bone defect to be replaced or restored plus 20%, 10%, 5% or 3%.

According to one embodiment, the implant molding system further comprises a molding
20 ring **3** cooperating with the mold **2** as shown in figure 3 and 4A. In the sense of the present invention cooperating refers to the fact that the molding ring **3** has a negative surface profile relative to the mold **2** such that joining the molding ring **3** with the mold **2** enable to guide the thickness and the edge of the implant.

According to one embodiment, the mold **2** has a surface larger than the bone-defect
25 thereby enabling the molding ring **3** to be positioned on the concave surface of the mold **2** and to define the thickness and the edge of the implant as shown in figure 4B.

According to one embodiment, the molding ring **3** has a thickness substantially equal to the thickness of the bone defect **1** at its periphery. According to one embodiment, the

inner contour of the molding ring **3** corresponds to the outer edge of the defect to be repaired or restored. According to one embodiment, when the molding ring **3** is placed in a concave mold **2**, the molding ring **3** cooperates with the mold **2** and forms a rim oriented towards the concavity of the mold **2**. According to one embodiment, when the implant forming material is pressed and shaped in the mold **2**, the molding ring **3** ensures correct shaping of the implant forming material (i.e. with the right thickness and outer size) as shown in figure 5A and 5B.

According to one embodiment, the molding ring **3** is designed via medical imaging. It may be manufactured by additive manufacturing. According to one embodiment, the molding ring **3** is patient-specific. According to one embodiment, the molding ring **3** is manufactured preoperatively. According to one embodiment, the molding ring **3** is manufactured per-operatively.

According to one embodiment, the implant is made by an implant molding system comprising a mold **2**, the tangible means for retaining the implant forming material in the mold **2** during hardening and for unmolding the hardened implant and a forming tool. According to one embodiment, the implant is made by an implant molding system comprising a mold **2**, the tangible means for retaining the implant forming material in the mold **2** during hardening and for unmolding the hardened implant and a counter mold **4**, **5**.

According to one embodiment, the implant molding system further comprises a forming tool having a negative surface profile relative to the mold **2**, such that joining the forming tool with the mold **2**, and optionally with the molding ring **3**, forms a cavity. Said cavity corresponds substantially to the shape of the defect **1** to be repaired.

According to one embodiment, the forming tool is used temporarily to shape the implant forming material.

According to one embodiment, the forming tool ring is designed via medical imaging. It may be manufactured by 3D printing technology. According to one embodiment, the forming tool **3** is patient-specific. According to one embodiment, the forming tool is

manufactured preoperatively. According to one embodiment, the forming tool is manufactured per-operatively.

According to one embodiment, the counter mold **4**, **5** is used temporarily to shape the implant forming material, especially its thickness.

- 5 According to one embodiment a counter mold **4** is used in the first steps of the implant molding process to facilitate the filing by the implant forming material in liquid phase within the mold **2**. As the implant forming material in liquid phase paste quickly, assuring a better filling by avoiding air bubbles is necessary and is realized by the use of a divided counter mold **4**. According to one embodiment, the counter mold **4** is divided into two
- 10 portions to permit, during assembly of the two parts filled with the implant forming material in liquid phase overflowing, producing enough pressure to ensure a good contact for a better implant quality.

- According to one embodiment, the implant molding system further comprises a counter mold **4**. According to one embodiment, the implant molding system does not comprise a
- 15 molding ring **3**. According to one embodiment, the counter mold **4** is a divisible counter mold **4** including a first counter mold portion **41** and a second counter mold portion **42**. According to one embodiment and represented in figure 6, each of the said counter mold portion is defined by two parts: an outer part, **412** and **422**, and an inner part, **411** and **421**. According to one embodiment, each part of the counter mold portion comprises outer
- 20 faces, **4112**, **4122**, **4222** and **4212**, and inner faces, **4111**, and **4211**, inner faces are oriented towards molding and outer faces are oriented towards outward. The said inner faces of the first **41** and second **42** counter mold portions outer parts, **412** and **422**, are shaped for receiving the mold **2**.

- According to one embodiment, the said outer parts, **412** and **422**, of the counter mold
- 25 portions, **41** and **42**, comprise a housing for the mold handle **23**. According to one embodiment and represented in figure 7, the said outer parts, **412** and **422**, of the counter mold portions, **41** and **42**, comprise a hole when gathered for the mold handle **23** to pass through. According to one embodiment, the said outer parts, **412** and **422**, of the counter mold portions, **41** and **42**, don't have a hole.

According to one embodiment, the mold **2** comprises a handle **23** on its outer face **21**. According to one embodiment, the mold **2** includes two mold portions to form a mold **2** with a concave shape on its inner face **22** when mated together, a first mold portion **24** and a second mold portion **25**. According to one embodiment, the first mold portion **24** has a first mold portion handle **241** and the second mold portion **25** has a second mold portion handle **251**. According to one embodiment, the first mold portion handle **241** and the second mold handle **251** comprise at least one fixing system to hold the two mold portions, **24** and **25**, together. According to one embodiment, the first **24** and the second **25** mold portion comprise a fixing system to hold the two mold portions together.

10 According to one embodiment, the said inner face of the implant is placed within the subject body and the said outer face of the implant is placed on the surface of the subject body.

According to one embodiment, the inner faces of the outer parts, **412** and **422**, of the first **41** and second **42** counter mold portions have a shape that interlock with the outer face **21** of the mold **2**. According to one embodiment, the inner faces of the outer parts of the first **41** and second **42** counter mold portions are fixed to the outer face **21** of the mold **2** by a binding agent such as glue. According to one embodiment, the external face of implant has a shape defined by the shape of the inner face **22** of the mold **2** and the shape of the internal face of the implant is defined by the shape of the inner faces of the inner parts, **411** and **421**, of the first **41** and second **42** counter mold portions, **4111** and **4211**.

According to one embodiment, the outer faces of the inner parts, **411** and **421**, of the first **41** and second **42** counter mold portions have a particular shape such as a planar or a concave surface. According to one embodiment, the outer faces of the inner parts, **411** and **421**, of the first **41** and second **42** counter mold portions, **4112** and **4212**, have a random shape.

According to one embodiment and as represented in figures 8A and 8B, the inner **411** and outer **412** parts of the first counter mold portion **41** comprise at least one fixing system **413** to hold them together. According to one embodiment, the fixing system **413** renders the said inner **411** and outer **412** parts of the first counter mold portion **41** dependent.

According to this embodiment, the first counter mold portion **41** comprises the first mold portion **24**.

According to one embodiment, the said inner **421** and outer **422** of the second counter mold portion **42** comprise at least one fixing system **423** to hold them together. According to one embodiment, the fixing system **423** renders the said inner **421** and outer **422** parts of the second counter mold portion **42** dependent. According to this embodiment, the second counter mold portion **42** comprises the second mold portion **25**.

According to one embodiment, the inner parts, **411** and **421**, of the first **41** and second **42** counter mold portions comprise at least one fixing system **43** represented in figures 9A and 9B. According to one embodiment, the fixing system **43** between the two inner parts, **411** and **421**, of the first **41** and second **42** counter mold portions can be defined as interlocking elements.

According to one embodiment, the two mold portions, **24** and **25**, and the four parts, **411**, **412**, **421** and **422**, of the counter mold **4** form a cavity localized between the inner face **22** of the mold **2** and the inner faces, **4111** and **4211**, of the inner parts, **411** and **421**, of the counter mold **4**.

According to another embodiment, as depicted in figures 10A, 10B, 10C and 10D, the counter mold **5** comprises a first portion **51** and a second portion **52**. According to one embodiment a counter mold **5** is used in the first steps of the implant molding process to facilitate the filing by the implant forming material of the mold **2**. According to one embodiment, the counter mold **5** and the mold **2** form, when mated together, a cavity corresponding to the image of the bone defect.

According to one embodiment, the first portion **51** comprises a hole for the mold handle **23** to pass through. According to one embodiment, the first portion **51** comprises a part exhibiting a predefined curvature corresponding to the curvature of the mold **2** and the second portion **52** comprises a part exhibiting a negative surface profile relative to the mold **2**. According to one embodiment, the first portion **51** and the second portion **52** are hinged together, preferably on one side by a revolute joint, such that when the implant forming material is deposited on the mold located within the counter mold **5**, and when

the first portion and the second portion **51**, **52** are mated together, the implant forming material is pressed homogeneously on the mold **2**.

According to one embodiment, the counter mold **4**, **5** is designed via medical imaging. It may be manufactured by 3D printing technology. According to one embodiment, the counter mold **4**, **5** is patient-specific. According to one embodiment, the counter mold **4**, **5** is manufactured preoperatively. According to one embodiment, the counter mold **4**, **5** is manufactured per-operatively.

According to one embodiment, the mold **2** and/or the molding ring **3** and/or the forming tool and/or the counter mold **4**, **5** is made of a biocompatible material. According to one embodiment, the mold **2** and/or the molding ring **3** and/or the forming tool and/or the counter mold **4**, **5** is made of ceramics, metals, metal alloys, glasses, polymers, bone or Portland like cement, gypsum, sand, stem cells or mixture thereof. According to one embodiment, the material of the mold **2** and/or the molding ring **3** and/or the forming tool and/or the counter mold **4**, **5** is selected from any materials suitable for additive manufacturing known by one skilled in the art. According to one embodiment, the mold **2** is a composite element comprising reinforcing element such as for instance metals, glasses or carbon fibers.

In one embodiment, the material of the mold **2** and/or the molding ring **3** and/or the forming tool and/or the counter mold **4**, **5** is selected from the group of polymer; preferably from the group of homopolymer or copolymer comprising polyamide (PA), poly(lactic acid) (PLA), poly(styrene), poly(butadiene) or poly(acrylonitrile); more preferable the mold material is selected from aliphatic polyamide such as but not limited to polycaprolactame (PA6), polylauroamide (PA12), polyundecanamide (PA11), polytetramethylene adipamide (PA4.6), polyhexylmethylen adipamide (PA6.6), polyhexylmethylen nonanediamide (PA6.9), polyhexylmethylen decanamide (PA6.10), polyhexylmethylen dodecanamide (PA6.12), polydecamethylen decanamide (PA10.10), polydecamethylen dodecanamide (PA10.12); semi-aromatic polyamide or polyphthalimide such as but not limited to polyhexylmethylen isophthalamide (PA 6.I), polyhexylmethylen terephthalamide (PA 6.T), polymetaxylene adipamide (PA mXD.6); aromatic polyamide or aramides such as but not limited to polymetaphenylene

isophthalamide (PA MPD.I) and polyparaphenylene terephthalamide (PA PPD.T). In one embodiment, the mold **2** and/or the molding ring **3** and/or the forming tool and/or the counter mold **4,5** is made of High Impact Poly(styrene) (HIPS). In one embodiment, the mold **2** and/or the molding ring **3** and/or the forming tool and/or the counter mold **4, 5** is made of a poly(acrylonitrile-*co*-butadiene-*co*-styrene) (ABS). In one embodiment, the mold **2** and/or the molding ring **3** and/or the forming tool and/or the counter mold **4, 5** is made of poly(etheretherketone) (PEEK). In one embodiment, the mold **2** and/or the molding ring **3** and/or the forming tool and/or the counter mold **4,5** is made of polyamide, such as PA12 or PA2200 commercialized by E-MANUFACTURING SOLUTIONS. In one embodiment, the mold **2** and/or the molding ring **3** and/or the forming tool and/or the counter mold **4, 5** is made of poly(ethylene-*co*-butylene terephthalate).

In one embodiment, the material of the mold **2** and/or the molding ring **3** and/or the forming tool and/or the counter mold **4, 5** does not deform during hardening of the implant forming material. In one embodiment, the material of the mold **2** and/or the molding ring **3** and/or the forming tool and/or the counter mold **4, 5** is selected from the group of polymer having a glass-transition temperature (T_g) equal or higher than the room temperature.

In one embodiment, the material of the mold **2** and/or the molding ring **3** and/or the forming tool and/or the counter mold **4, 5** is selected from the group of polymer having a melting temperature (T_m) higher than the reaction temperature. In one embodiment, the material of the mold **2** and/or the molding ring **3** and/or the forming tool and/or the counter mold **4, 5** is selected from the group of polymer having a glass temperature (T_g) lower than the reaction temperature. In one embodiment, the material of the mold **2** and/or the molding ring **3** and/or the forming tool and/or the counter mold **4, 5** is selected from the group of polymer having a melting temperature (T_m) higher than 45°C, preferably higher than 70°C, more preferably higher than 90°C, even more preferably higher than 110°C. In one embodiment, the melting temperature (T_m) is at least 50°C higher than the reaction temperature of the implant.

According to one embodiment, the material of the mold **2** and/or the molding ring **3** and/or the forming tool and/or the counter mold **4,5** resists (*i.e.* does not deform if exposed) to

temperatures higher than room temperature; preferably higher than 40°C; more preferably higher than 90°C. In one embodiment, the material of the mold **2** and/or the molding ring **3** and/or the forming tool resists to temperature around 90°C. In one embodiment, the material of the mold **2** and/or the molding ring **3** and/or the forming tool and/or the counter mold **4,5** resists to temperature about 135°C. According to one embodiment, said temperature is achieved by an external source of heat.

According to one embodiment, the material of the forming tool is selected from homopolymer or copolymer of polysiloxan (also called silicone).

The implant molding system of the present invention also comprises means for retaining the implant forming material in the mold **2** during hardening and for unmolding the hardened implant thereafter. According to one embodiment, said means is a coating.

According to one embodiment, the mold **2** of the invention is larger than the bone defect **1** of a patient such that the mold rests on the existing bone around the defect **1** during testing by the surgeon; thereby providing the surgeon the ability to modify the implant geometry depending on the size of the opening performed to repair or restore the bone defect **1**. In order to ensure that when testing the implant *in situ*, the curvature is conserved, the surgeon holds the implant within the mold. The adhesion between the implant forming material and the mold **2** must thus be sufficient in order to avoid deformation or loss of the implant during testing and should also enable unmolding without deformation after hardening. When unmolding is required after hardening of the implant forming material, the adhesion between the implant molding material and the mold **2** should also be sufficiently weak to ensure unmolding without structural deformation and cross-contamination. To that end, the implant molding system of the invention comprises means for retaining the implant forming material in the mold **2** during hardening and for unmolding the hardened implant. Said means also avoid contamination of the implant forming material by the material of the mold **2**.

According to one embodiment, the means for ensuring adhesion between the implant forming material and the mold **2** during hardening and for unmolding the hardened implant is a coating.

According to one embodiment, said coating allows: 1) ensuring adhesion between the hardening implant material and the mold **2** during hardening; and 2) ensuring easy unmolding after hardening of the implant while avoiding contamination of said implant by the material of the mold **2**.

- 5 According to one embodiment, said adhesion is sufficient to retain the implant forming material in the mold even if the concave surface of the mold **2** is directed downwards during 2, 3, 4, 5 or 10 minutes.

- Consequently, said coating retains the implant forming material against gravity and potential forces during implant forming material application and during adaptation, e.g.
10 on the patient.

According to one embodiment, in a first state said coating ensures that the implant forming material stays on the mold and in a second state, said coating enables easy unmolding of the implant from the mold.

- According to one embodiment, the ability of implant unmolding depends on the reduction
15 of the physical adhesion between the implant and the mold **2** material.

According to one embodiment, once applied on the surface of the mold **2**, at room temperature or at a temperature ranging from 0 to 30°C, preferably from 15 to 25°C, the coating forms a solid or viscous layer.

- According to one embodiment, the coating is selected from vaseline, or Horsley's wax or
20 homopolymer or copolymer of poly(isoprene), poly(chloroprene), poly(vinyl alcohol), poly(acrylonitrile), poly(butadiene), poly(vinyl chloride), poly(ethylene), poly(isobutylene), poly(ethylene glycol), poly(lactic acid) or any mixtures thereof.

According to one embodiment, the coating is applied on the surface of the mold **2** in a liquid or viscous form.

- 25 According to one embodiment, the coating is a biocompatible compound. According to one embodiment, the coating is a bioresorbable compound.

In one embodiment, the coating is selected from biocompatible polymer selected from functionalized or unfunctionalized poly(ethylene glycol), preferably PEG 1000 or PEG 1500. PEG 1000 and PEG 1500 have the advantage of being sticky in solid form. In such a manner, it ensure retention between the mold and the implant forming material in the mold **2** during hardening due to physical adhesion between the implant forming material and the PEG. When the PEG is liquid, it does not ensure retention and the implant can be easily unmold from the mold. In one embodiment, the coating is a homopolymer or copolymer comprising poly(ethylene glycol) moiety. In one embodiment, the coating is a biocompatible lubricant such as but not limited to petroleum jelly (vaseline), natural or synthetic oil, waxes such as Horsley's wax or bone wax, macroproteins such as gelatin, glucid such as sugar or starch. In one embodiment, the coating is selected from biocompatible polymer selected from poly(lactic acid).

In one embodiment, the coating is selected from Horsley's wax or vaseline or homopolymer or copolymer of poly(ethylene glycol) or any mixtures thereof.

15 In one embodiment, the coating is selected from a biocompatible polymer having a molar weight ranging from 130 g/mol to 1 000 000 g/mol; preferably ranging from 500 g/mol to 800 000 g/mol; more preferably ranging from 800 to 10 000 g/mol. In one embodiment, the coating is a biocompatible polymer having a molar weight of about 1 000 g/mol.

According to one embodiment, in order to apply the coating on the mold **2**, the coating is solubilized with at least one solvent such as for instance water, alcohol, acetone or chlorinated solvents. According to an embodiment, a diluted solution of the coating is applied on the mold **2**. In one embodiment, the solution comprising a coating may further comprise a dye and/or pigment and/or an antibiotic. In one embodiment, the solvent is human-safe. In one embodiment, the solvent may be easily evaporated after deposition on the mold **2**.

According to one embodiment, the coating is melt before application. According to one embodiment a molten coating is applied on the mold **2** and then cooled until it forms a solid layer, before application of the implant forming material.

According to one embodiment, the coating also comprises a dye.

According to one embodiment, the coating is selected from the group of polymer having a melting temperature ($T_{m \text{ coating}}$) higher than T_1 and lower than T_2 , wherein T_1 is the room temperature and T_2 is the reaction temperature of the implant manufacture.

5 According to one embodiment, the coating is selected from the group of polymer having a melting temperature ($T_{m \text{ coating}}$) higher than T_1 and lower than T_2 , wherein T_1 is ranging from 0 to 40°C, preferably from 25 to 40°C, more preferably about 40°C and T_2 is ranging from 45 to 100°C, preferably from 70 to 90°C, more preferably about 60°C.

10 In one embodiment, the coating is selected from the group of polymer having a phase transition at a temperature higher than T_1 and lower than T_2 , wherein T_1 is ranging from 0 to 40°C, preferably from 25 to 40°C, more preferably about 40°C and T_2 is ranging from 45 to 100°C, preferably from 70 to 90°C, more preferably about 60°C.

15 In one embodiment, the coating is selected from the group of polymer having a phase transition temperature ranging from 40 to 100°C, from 40 to 90°C, from 40 to 80°C, from 40 to 70°C, from 40 to 65°C or from 45 to 60°C. In said embodiment, the phase transition temperature does not refer to the glass-transition temperature.

In one embodiment, the coating is selected from the group of polymer having a melting point from 45 to 60°C, from 40 to 100°C, from 40 to 90°C, from 40 to 80°C, from 40 to 70°C, from 40 to 65°C or from 45 to 60°C.

20 In one embodiment, the coating is viscous or solid at ambient temperature and is liquid at the reaction temperature of the implant manufacture.

According to one embodiment, the coating in liquid or viscous form is deposited on the mold by any means known by one skilled in the art such as for instance thermoforming, spray-coating, dip-coating, painting, spin-coating or calendering.

25 According to one embodiment, the coating ensures retention of the implant forming material in the mold **2** during hardening due to physical adhesion between the implant forming material and the coating. According to one embodiment, the coating ensures unmolding of the hardened implant due to the temperature of the exothermic reaction of hardening of the implant forming material which exceed the melting temperature of the

coating. According to an alternative embodiment, the coating ensures unmolding of the hardened implant due to the heating of the coating by means of an external heat source at a temperature above the melting temperature of the coating.

According to one embodiment, the coating is applied on the surface of the mold **2** in a
5 solid or viscous form.

According to one embodiment, the coating ensures retention of the implant forming material in the mold **2**. After the coating turns into a liquid form, it does not ensure retention anymore and ensures unmolding of the hardened implant.

According to one embodiment, the coating is applied in the form of a solid film.
10 According to one embodiment, the solid film is made of biocompatible polymer. In one embodiment, the solid film is a polymer selected from homopolymer or copolymers of poly(isoprene), poly(chloroprene), poly(vinyl alcohol), poly(acrylonitrile), poly(butadiene), poly(vinyl chloride), poly(ethylene), poly(isobutylene); preferably is a poly(acrylonitrile-*co*-butadiene).

15 According to an embodiment, the solid film is selected from pressure-sensitive tape or nitrile butadiene rubber.

According to one embodiment, once applied on the mold **2**, the solid film comprises a tab extending outside of the mold **2** enabling peeling said coating off the mold **2**. According to one embodiment, once applied on the mold **2**, the solid film comprises a tab extending
20 outside of the mold **2** enabling peeling said coating and the implant off the mold **2**.

According to one embodiment, the solid film ensures retention of the implant forming material in the mold **2** during hardening due to physical adhesion between the implant forming material and the solid film. According to one embodiment, the solid film ensures unmolding of the hardened implant by peeling said film off the mold **2**.

25 According to one embodiment, the implant forming material is selected from any implant forming material known by one skilled in the art such as for instance Palacos® or Palamed® commercialized by Heraeus.

According to one embodiment, the implant forming material is selected from biocompatible materials suitable for class IIb or class III medical devices. In one embodiment, the implant comprises a cross-linked polymer. In one embodiment, the implant does not comprise any cross-linked polymer.

- 5 According to one embodiment, the implant forming material mainly comprises a material having a glass-transition temperature higher than 40°C; preferably higher than 90°C. In one embodiment, the implant mainly comprises a material having a glass-transition temperature about 110°C.

According to one embodiment, the implant forming material of the implant molding
10 system comprises a composition comprising the mixture of a liquid phase comprising:

- at least one liquid monomer; and
- at least one polymerization inhibitor;

and a solid phase comprising:

- at least one polymer;
- 15 - at least one initiator;
- optionally at least one activator; and
- optionally at least one radio-opaque filler.

According to one embodiment, the liquid monomer is selected from the group of acrylates, methacrylates, styrenics, acrylamides, amides, urethanes, amino acids such as
20 but not limited to lactic acid; preferably selected from the group of acrylates, methacrylates or combination thereof; more preferably the monomer is methyl methacrylate. In one embodiment, the liquid monomer is methyl methacrylate.

According to one embodiment, the polymerization inhibitor is hydroquinone.

According to one embodiment, the liquid phase further comprises at least one dye and/or
25 pigment selected from at least one biocompatible dye and/or pigment; more preferably from food additives. In one embodiment, the liquid phase further comprises additive copper complexes of chlorophylls (E141).

According to one embodiment, the polymer powder comprises homopolymer or copolymer obtained by the polymerization of at least one monomer selected from the group of acrylates, methacrylates, styrenics, acrylamides, amides, urethanes, amino acids such as but not limited to lactic acid; preferably selected from the group of acrylates, methacrylates or combination thereof; more preferably the polymer powder is a
 5 copolymer of methyl methacrylate and methyl acrylate.

In one embodiment the polymer powder comprises random, block, linear, dendritic, branched, cross-linked polymer or combination thereof.

According to one embodiment, the initiator is selected from a photoinitiator, a radical
 10 initiator or a redox initiator; preferably from a diazoinitiator, such as azobisisobutyronitrile (AIBN), 2,2'-azobis(2-methylpropionamidine); a peroxide, such as acyl peroxides, acetyl peroxides, benzoyl peroxides, alkyl peroxides, hydroperoxides, acyl alkylsulfonyl peroxides, dialkyl peroxydicarbonates, diperoxyketals, ketone peroxides; a perester; an azo; a disulfide; a tetrazene; a persulfate compounds.

15 In one embodiment, the initiator is benzoyl peroxide.

According to one embodiment, the photoinitiator is selected from 2-tert-butylanthraquinone; camphorquinone; diphenyl(2,4,6-trimethylbenzoyl)phosphine oxide; 9,10-phenanthrenequinone; phenylbis(2,4,6-trimethylbenzoyl)phosphine oxide; 2-benzyl-2-(dimethylamino)-4'-morpholinobutyrophenone; 3,6-bis(2-methyl-2-morpholinopropionyl)-9-octylcarbazole; 4'-tert-butyl-2',6'-dimethylacetophenone; 2,2-diethoxyacetophenone; 4'-ethoxyacetophenone; 3'-hydroxyacetophenone; 4'-hydroxyacetophenone; 1-hydroxycyclohexylphenylcetone; 2-hydroxy-4'-(2-hydroxyethoxy)-2-methylpropiophenone; 2-hydroxy-2-methylpropiophenone; 2-methyl-4'-(methylthio)-2-morpholinopropiophenone; 4'-phenoxyacetophenone; benzoin;
 20 benzoinethyl ether benzoinmethyl ether; 4,4'-dimethylbenzoin, 4,4'-dimethylbenzil; benzophenone; benzoylbiphenyl; 4,4'-bis(diethylamino)benzophenone; 4,4'-dihydroxybenzophenone; 3,4-dimethylbenzophenone; 3-hydroxybenzophenone; 4-hydroxybenzophenone; 2-methylbenzophenone; 3-methylbenzophenone; 4-methylbenzophenone; methylbenzoylformate; Michler ketone; 1-chloro-4-propoxy-9H-

thioxanthen-9-one; 2-chlorothioxanthen-9-one; 2,4-diethyl-9H-thioxanthen-9-one; isopropyl-9H-thioxanthen-9-one; 10-methylphenothiazin; thioxanthen-9-one; preferably from 2,4-dihydroxybenzophenone, ethyl 4-dimethylaminobenzoate and camphorquinone.

- 5 According to one embodiment, the solid phase comprises at least one activator such as for instance N,N-dimethyl-p-toluidine.

According to one embodiment, the solid phase comprises at least one radio-opaque filler such as for instance zirconium dioxide.

- 10 According to one embodiment, the solid phase further comprises at least one dye and/or pigment selected from at least one biocompatible dye and/or pigment; more preferably the at least one dye and/or pigment is selected from food additives. In one embodiment, the solid phase further comprises additive copper complexes of chlorophylls (E141).

According to one embodiment, the solid phase further comprises at least one antibiotic such as for instance gentamicin.

- 15 According to one embodiment, the composition is hardened by the mixture between the solid phase and the liquid phase. In one embodiment, the hardener is the initiator.

In one embodiment, the mixture between the solid phase and the liquid phase is carried out in the open air. In one embodiment, the mixture between the solid phase and the liquid phase is carried out under inert gas.

- 20 In one embodiment, the mixture between the solid phase and the liquid phase leads to a homogeneous paste. In one embodiment, the mixture between the solid phase and the liquid phase leads to a sticky paste. In one embodiment, the mixture between the solid phase and the liquid phase leads to a paste with good handling properties.

- 25 The invention also relates to a process for manufacturing the coated implant molding system comprising the following steps:

— providing:

- a mold **2** having a surface concave along at least one axis obtained by additive manufacturing from medical imaging;
- optionally, a molding ring **3** obtained by additive manufacturing from medical imaging;
- 5 – optionally, a forming tool obtained by additive manufacturing from medical imaging; and
- means for retaining the implant forming material in the mold **2** during hardening and for unmolding the hardened implant; and
- coating the concave surface of the mold **2** with the means for retaining the implant forming material in the mold **2** during hardening and for unmolding the hardened implant thereafter.

The invention also relates to a process for manufacturing the implant comprising the following steps:

- providing:
- 15 – a mold **2** having a surface concave along at least one axis obtained by additive manufacturing from medical imaging;
- optionally, a molding ring **3** obtained by additive manufacturing from medical imaging;
- optionally, a forming tool obtained by additive manufacturing from medical imaging;
- 20 – an implant forming material comprising a composition comprising a liquid phase comprising at least one monomer and at least one polymerization inhibitor; and a solid phase comprising at least one polymer, at least one initiator, at least one activator and at least one radio-opaque filler; and
- 25 – means for retaining the implant forming material in the mold **2** during hardening and for unmolding the hardened implant; and
- coating the concave surface of the mold **2** with the means for retaining the implant forming material in the mold **2** during hardening and for unmolding the hardened implant thereafter;

- mixing the liquid phase comprising at least one liquid monomer and at least one polymerization inhibitor; with the solid phase comprising at least one polymer, at least one initiator, at least one activator; and at least one radio-opaque filler;
- shaping the implant forming material by spreading out the implant forming material onto the concave surface of the mold **2**; optionally by means of the molding ring **3** and/or the forming tool;
- hardening of the implant during a setting time;
- unmolding the implant from the mold **2**;
- optionally heating the implant by means of an external heat source;
- adapting the implant by making holes or the like.

According to one embodiment, in order to avoid residual monomers, post-hardening heating is achieved preferably up to 95, 90, 85, 80 or 75°C during 5, 10, 15, 20, 30, 45 or 60 minutes.

According to one embodiment, post heating is achieved preferably up to 90°C during 15 minutes.

According to one embodiment, the process is exothermic. According to one embodiment, if the process is not exothermic the heat source is provided by an external source.

According to one embodiment, the implant forming material is spread out in the mold **2**, and optionally in the molding ring **3**, and is pressed to be shaped.

According to one embodiment, the implant forming material is pressed using a forming tool having a negative surface profile relative to the mold **2**, such that joining the forming tool with the mold **2**, and optionally with the molding ring **3**, forms a cavity having the shape and thickness of the defect.

According to one embodiment, the implant forming material may be shaped (shaping time) between 30 seconds and 15 minutes after mixing the solid phase and the liquid phase of the implant forming material, preferably between 1 and 12 minutes, more preferably between 1 and 7 minutes. According to one embodiment, in order to extend

the shaping time, the liquid and solid phases of the implant forming material are cooled down before mixing.

According to one embodiment, the setting time is ranging from 5 to 30 minutes, preferably from 10 to 15 minutes.

5 The invention also relates to a process for manufacturing the implant comprising the following steps:

- providing:
 - a mold **2** having a surface concave along at least one axis obtained by additive manufacturing from medical imaging, the said mold **2** is divided
10 in a first **24** and a second **25** mold portions;
 - a counter mold **4,5** divided in two counter mold portions : the first **41** and the second **42** counter mold portions, wherein each of the portion is divided in two parts : the inner, **411** and **421**, and the outer parts, **412** and **422**; when the four parts are mated together the counter mold **4** comprises
15 a cavity correspondingly shaped with the mold **2** and the desired implant;
 - an implant forming material comprising a composition comprising a liquid phase comprising at least one monomer and at least one polymerization inhibitor; and a solid phase comprising at least one polymer, at least one initiator, at least one activator and at least one radio-opaque filler; and
- 20 – coating the concave surface of the mold **2** with the means for retaining the implant forming material in the mold **2** during hardening and for unmolding the hardened implant thereafter;
- fixing the first mold portion **24** onto the inner face of the outer part **412** of the first counter mold portion **41** optionally by means of binding agent;
- 25 – assembling the inner part **411** and the outer part **412** of the first counter mold portion **41** by means of at least one fixing system, wherein the first mold portion **24** is fixed, by means of at least one fixing system;
- fixing the second mold portion **25** onto the inner face of the outer part **422** of the second counter mold portion **42** optionally by means of binding agent;

- assembling the inner part **421** and the outer part **422** of the second counter mold portion **42**, wherein the second mold portion **25** is fixed, by means of at least one fixing system;
- mixing the liquid phase comprising at least one liquid monomer and at least one polymerization inhibitor; with the solid phase comprising at least one polymer, at least one initiator, at least one activator; and at least one radio-opaque filler;
- shaping the implant forming material by pouring the implant forming material into the cavity of the first **41** and of the second **42** counter mold portions;
- assembling the first **41** and second **42** counter mold portions by means of at least one fixing system **43**;
- hardening of the implant during a setting time;
- disassembling the counter mold **4,5** to release the mold **2** filled by the implant forming material;
- optionally heating the implant by means of an external heat source;
- adapting the implant by making holes or the like.

According to one embodiment, in order to avoid residual monomers, post-hardening heating is achieved preferably up to 95, 90, 85, 80 or 75°C during 5, 10, 15, 20, 30, 45 or 60 minutes.

According to one embodiment, post heating is achieved preferably up to 90°C during 15 minutes.

According to one embodiment, the process is exothermic. According to one embodiment, if the process is not exothermic the heat source is provided by an external source.

According to one embodiment, the implant forming material may be shaped (shaping time) between 30 seconds and 15 minutes after mixing the solid phase and the liquid phase of the implant forming material, preferably between 1 and 12 minutes, more preferably between 1 and 7 minutes. According to one embodiment, in order to extend the shaping time, the liquid and solid phases of the implant forming material are cooled down before mixing.

According to one embodiment, the setting time is ranging from 5 to 30 minutes, preferably from 10 to 15 minutes.

The invention also relates to a cranioplasty method of a subject comprising the following steps:

- 5 – providing:
 - a mold **2** having a surface concave along at least one axis obtained by additive manufacturing from medical imaging;
 - optionally, a molding ring **3** obtained by additive manufacturing from medical imaging;
- 10 – optionally, a forming tool obtained by additive manufacturing from medical imaging;
- an implant forming material comprising a composition comprising a liquid phase comprising at least one monomer and at least one polymerization inhibitor; and a solid phase comprising at least one polymer, at least one initiator, at least one activator and at least one radio-opaque filler; and
- 15 – means for retaining the implant forming material in the mold **2** during hardening and for unmolding the hardened implant thereafter; and
- coating the concave surface of the mold **2** with the means for retaining the implant forming material in the mold **2** during hardening and for unmolding the hardened implant thereafter;
- 20 – mixing the liquid phase comprising at least one liquid monomer and at least one polymerization inhibitor; with the solid phase comprising at least one polymer, at least one initiator, at least one activator; and at least one radio-opaque filler;
- shaping the implant forming material by spreading out the implant forming material onto the concave surface of the mold **2** and optionally by means of the molding ring **3** and/or the forming tool;
- 25 – testing the implant on the patient's skull after removal of the optional molding ring **3** and the optional forming tool during the shaping time;
- optionally, reshaping the implant;
- 30 – hardening of the implant during a setting time;

- unmolding the implant from the mold 2;
 - optionally heating the implant by means of an external source;
 - adapting the implant by making holes or the like;
 - placing the implant into the patient's skull; and
- 5 – fixing the implant into the patient's skull by means of fixation known by one skilled in the art.

According to one embodiment, the implant forming material may be shaped during a shaping time ranging from 30 seconds to 15 minutes after mixing the solid phase and the liquid phase of the implant forming material, preferably between 1 and 12 minutes, more
10 preferably between 1 and 7 minutes. According to one embodiment, in order to extend the shaping time, the liquid and solid phases of the implant forming material are cooled down before mixing.

According to one embodiment, the setting time is ranging from 1 to 15 minutes or from 2 to 10 minutes or from 3 to 5 minutes.

- 15 According to one embodiment, in order to avoid residual monomers, post-hardening heating is achieved preferably up to 95, 90, 85, 80 or 75°C during 5, 10, 15, 20, 30, 45 or 60 minutes.

According to one embodiment, post heating is achieved preferably up to 90°C during 15 minutes.

- 20 According to one embodiment, the process is exothermic. According to one embodiment, if the process is not exothermic the heat source is provided by an external source.

According to one embodiment, the implant molding system is sterilized, for instance by autoclave, γ irradiation, ethylene oxide sterilization or gas plasma sterilization. According to one embodiment, the coating resists to sterilization processes such as but not limited
25 to EtO sterilization, γ irradiation, gas plasma sterilization; preferably is stable in autoclave.

The present invention has been described in terms of specific embodiments, which are illustrative of the invention and not to be construed as limiting. More generally, it will be appreciated by persons skilled in the art that the present invention is not limited by what has been particularly shown and/or described hereinabove.

5

BRIEF DESCRIPTION OF THE DRAWINGS

The foregoing summary and detailed description of the invention will be better understood when read in conjunction with the appended drawings. For the purpose of illustrating the invention, there are shown in the drawings, certain embodiments which
10 are presently preferred. It should be understood, however, that the invention is not limited to the precise arrangements and instrumentalities shown.

Figure 1 illustrates a bone defect **1** to be repaired or restored.

Figures 2A and **2B** illustrate a mold **2** according to one embodiment of the invention.

Figure 3 illustrates a bone defect **1** to be repaired or restored together with a molding ring
15 **3** and a mold **2** according to one embodiment of the invention. The mold **2** has the curvature of the bone defect **1** to be repaired or restored while the inner edge of the molding ring **3** has the thickness and shape of the bone defect **1** at its periphery.

Figures 4A and **4B** illustrate a mold **2** and a molding ring **3** according to one embodiment of the invention.

20 **Figures 5A** and **5B** illustrate a mold **2** according to one embodiment of the invention positioned in a bone defect **1** in order to test *in situ* the hardening implant.

Figure 6 illustrates a counter mold **4** divided into two parts and a mold **2** with a handle **23**.

Figure 7 illustrates an assembled counter mold **4** and a mold **2** with a handle **23**.

25 **Figures 8A** and **8B** illustrate an assembled counter mold **4** and a mold **2** with a handle **23** with a view from each face.

Figures 9A and 9B illustrate the two portions, **41** and **42**, of the counter mold **4** and mold **2** assembled wherein the cavity has the desired shape for the implant.

Figures 10A, 10B, 10C and 10D illustrate a counter mold **5** divided into two portions **51**, **52**.

- 5 The drawings are not drawn to scale and are not intended to limit the scope of the claims to the embodiments depicted.

REFERENCES

- 1 – Bone defect of a patient;
- 10 2 – Mold;
 - 21 – Outer face of the mold;
 - 22 – Inner face of the mold;
 - 23 – Handle;
 - 24 – First mold portion;
 - 15 241 – Handle;
 - 25 – Second mold portion;
 - 251 – Handle;
- 3 – Molding ring;
- 4 – Counter mold;
- 20 41 – First counter mold portion;
 - 411 – Inner part;
 - 4111 – Inner face;
 - 4112 – Outer face;
 - 412 – Outer part;
 - 25 4122 – Outer face;
 - 413 – Fixing systems;
- 42 – Second counter mold portion;
 - 421 – Inner part;
 - 4211 – Inner face;

- 4212 – Outer face;
- 422 – Outer part;
- 4222 – Outer face;
- 423 – Fixing systems;
- 5 43 – Fixing systems;
- 5 – Counter mold;
- 51 – First counter mold portion;
- 52 – Second counter mold portion.

10 EXAMPLE

The following example will be better understood when read in conjunction with the drawings.

- In order to confirm the ability of a PEG 1000-coating on a polyamide mold to resolve the adhesion and contamination issues, an implant has been manufactured according to the
- 15 present invention using the following steps:
- obtaining an image of a bone defect of a patient **1** by means of CT-scans, as represented in figure 1;
 - manufacturing a mold **2**, as represented in figures 2A and 2B, in polyamide (PA12) having the curvature of the bone defect **1** and a surface larger than the bone defect **1** itself
 - 20 by mean of 3D printing;
 - manufacturing a molding ring **3**, as represented in figure 3, in polyamide (PA12) wherein the inner edge of the molding ring **3** has the thickness and shape of the bone defect **1** at its periphery by mean of 3D printing;
 - heating a PEG 1000 composition at 80°C during 5 minutes in order to melt it;
 - 25 - impregnating a gauze with the melted PEG 1000 composition;
 - rubbing the impregnated gauze on the mold;
 - let the PEG 1000 coating hardened on the mold at room temperature during 5 minutes;
 - inserting/cooperating the molding ring **3** with the mold **2**, as illustrated in figures 4A and 4B;
 - 30 - shaping a Palacos[®] composition on the coated mold;

- let the implant hardened on the mold; as the hardening reaction is exothermic, the PEG 1000 coating shall melt; and
- demolding the implant from the mold.

According to one embodiment, during the shaping of the Palacos[®] composition, the
5 molding ring **3** may be removed from the mold **2** and the implant may be tested on the patient by means of the mold **2**, as illustrated in figures 5A and 5B.

CLAIMS

1. An implant molding system for the molding of an hardenable implant forming material comprising:
 - a mold (2) obtainable from an image of a bone defect (1) by additive manufacturing;
 - said mold (2) having a surface concave along at least one axis;the concave surface along at least one axis conforms to an arc with a radius ranging from 2 to 20 centimeters;
- the implant molding system further comprising tangible means for retaining the implant forming material, for instance against gravity, in the mold (2) during hardening and for unmolding the implant after hardening;
- said tangible means for retaining the implant forming material in the mold (2) during hardening and for unmolding after hardening comprises or consists of a coating, said coating being applied onto the concave surface of the mold (2);
- wherein said coating is made of a biocompatible material and said coating has a phase transition temperature ranging from 40 to 100°C.
2. The implant molding system according to claim 1, wherein said coating is selected from vaseline, or Horsley's wax or homopolymer or copolymer of poly(isoprene), poly(chloroprene), poly(vinyl alcohol), poly(acrylonitrile), poly(butadiene), poly(vinyl chloride), poly(ethylene), poly(isobutylene), poly(ethylene glycol), poly(lactic acid) or any mixtures thereof.
3. The implant molding system according to claim 1 or claim 2, wherein said coating forms a solid layer at a temperature ranging from 0 to 30°C, preferably from 15 to 25°C.
4. The implant molding system according to anyone of claims 1 to 3, wherein said coating is applied onto the concave surface of the mold (2) in solid form.
5. The implant molding system according to claim 4, wherein said coating further comprises a tab extending outside of the mold (2) enabling peeling said coating off the mold (2).

6. The implant molding system according to claim 4 or 5, wherein said coating is selected from poly(acrylonitrile-*co*-butadiene).
7. The implant molding system according to anyone of claims 1 to 3, wherein said coating is applied onto the concave surface of the mold (2) in liquid form.
- 5 8. The implant molding system according to claim 7, wherein the coating exhibits a melting temperature above T1 and below T2, wherein T1 is ranging from 0 to 40°C, preferably from 25 to 40°C and wherein T2 is ranging from ranging from 45 to 100°C, preferably from 70 to 90°C.
9. The implant molding system according to claim 7 or 8, wherein said coating is
10 selected from Horsley's wax or vaseline or homopolymer or copolymer of poly(ethylene glycol) or any mixtures thereof.
10. The implant molding system according to anyone of claims 1 to 9, further comprising a molding ring (3) having a negative surface profile relative to the mold (2), an inner edge and a predefined thickness along the edge.
- 15 11. The implant molding system according to anyone of claims 1 to 10, further comprising a forming tool having a negative surface profile relative to the mold (2), such that joining the forming tool with the mold, and optionally with the molding ring (3), forms a cavity.
12. The implant molding system according to anyone of claims 1 to 10, further
20 comprising a counter mold (4, 5) comprising a first and a second counter mold portion (41, 42, 51, 52), each comprising an inner part and an outer part, wherein the counter mold (4, 5) and the mold (2) form, when mated together, a cavity corresponding to the image of the bone defect.
13. The implant molding system according to anyone of claims 1 to 12, wherein the
25 surface concave along at least one axis conforms to an arc with a radius ranging from 4.5 to 9.5 centimeters, or substantially equal to 7 centimeters.

- 14.** The implant molding system according to anyone of claims **1** to **13**, wherein the mold (2) and/or the molding ring (3) and/or the forming tool comprises a material selected from ceramics, metals, metal alloys, glasses, polymers, bone or portland like cement, gypsum, sand or mixture thereof.
- 5 **15.** The implant molding system according to anyone of claims **1** to **14**, further comprising an hardenable implant forming composition comprising a liquid phase comprising at least one liquid monomer, and at least one polymerization inhibitor; and a solid phase comprising at least one polymer, at least one initiator, optionally at least one activator, and optionally at least one radio-opaque filler.

1/7

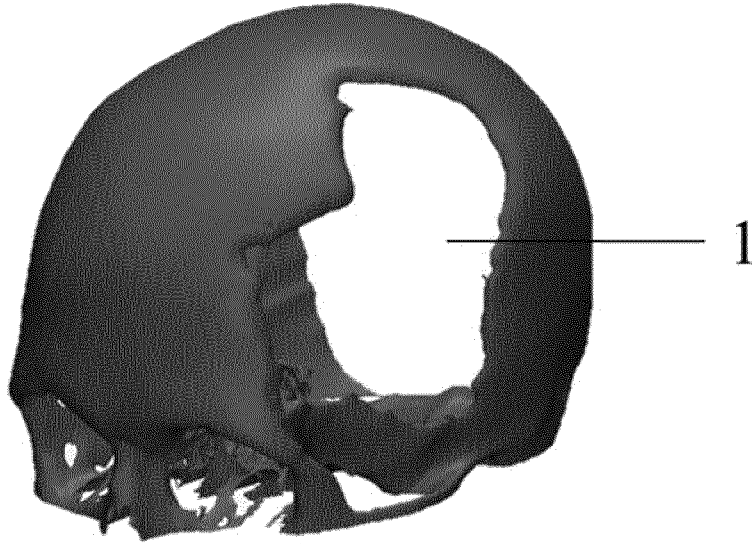


FIG. 1

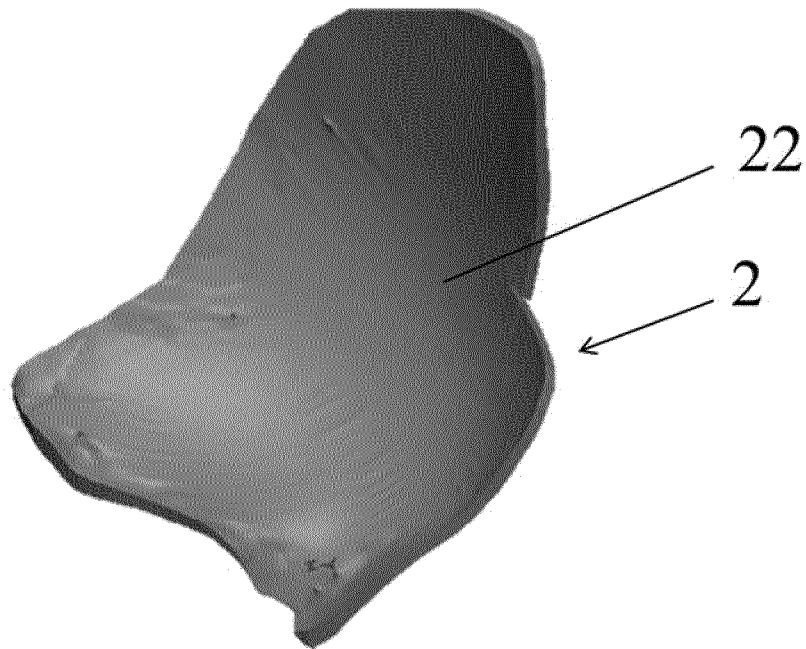


FIG. 2A

2/7

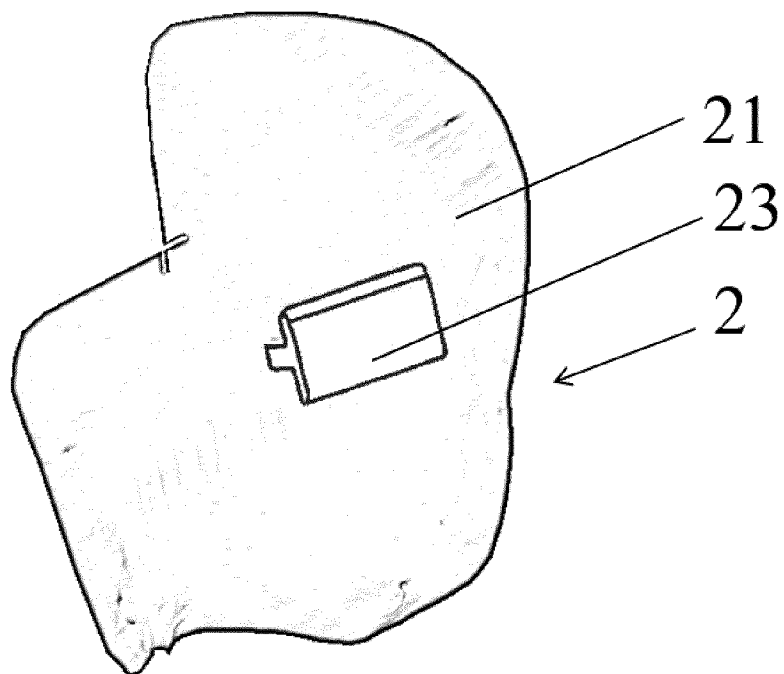


FIG. 2B

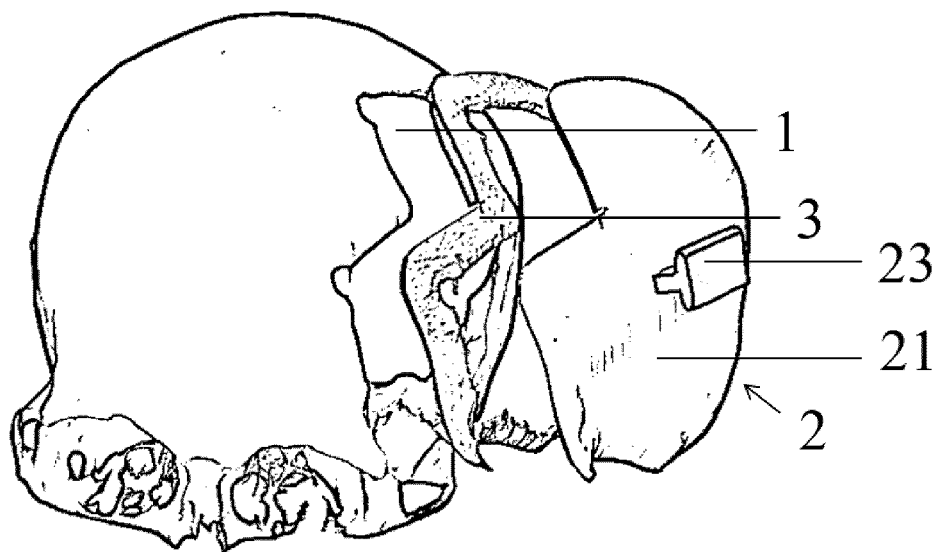


FIG. 3

3/7

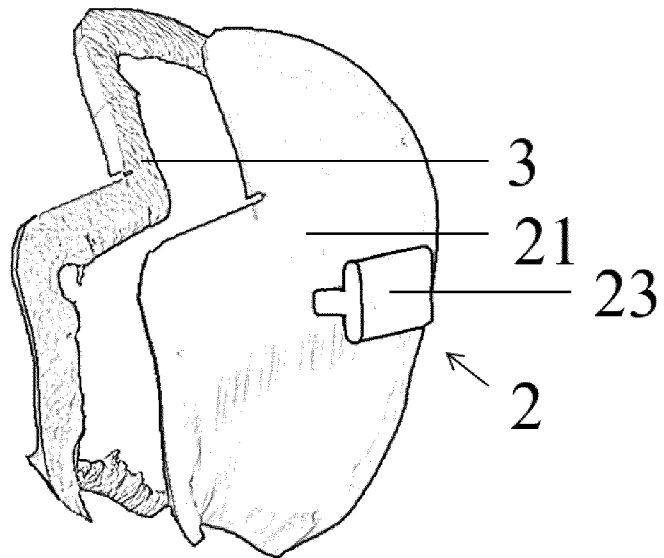


FIG. 4A

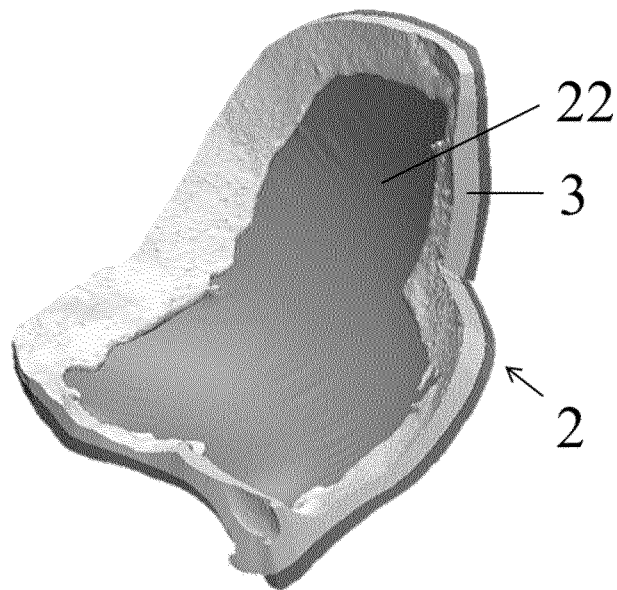


FIG. 4B

4/7

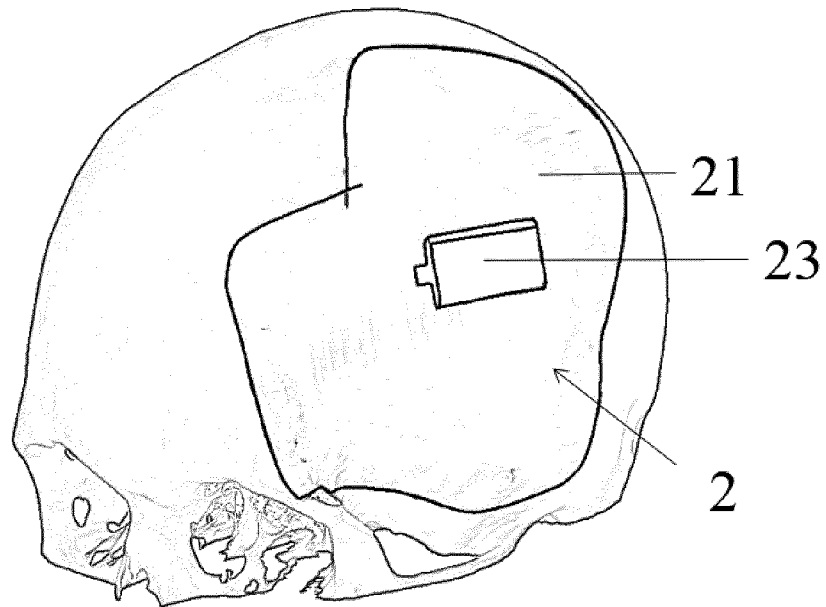


FIG. 5A

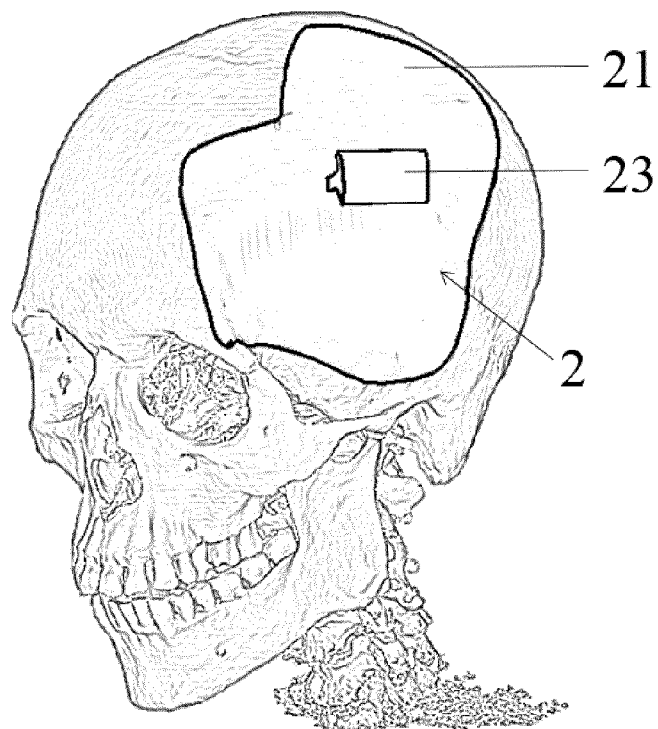


FIG. 5B

5/7

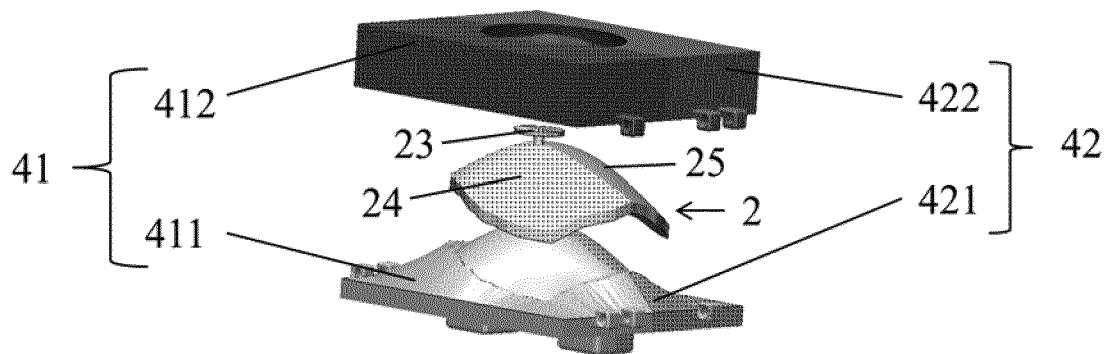


FIG. 6

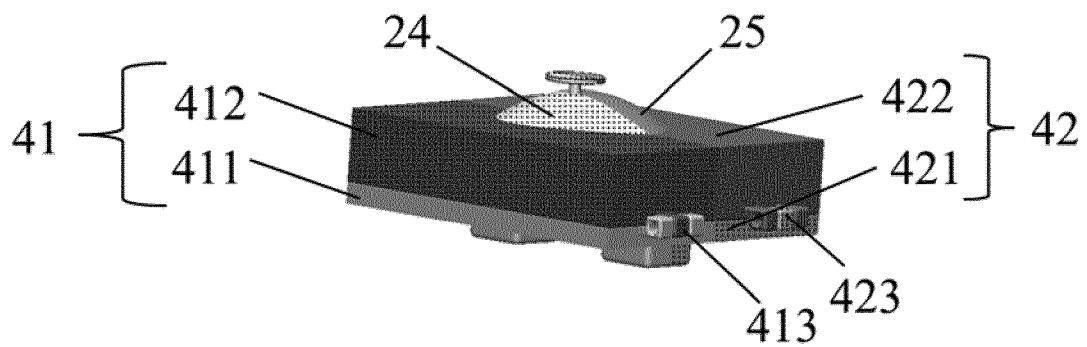


FIG. 7

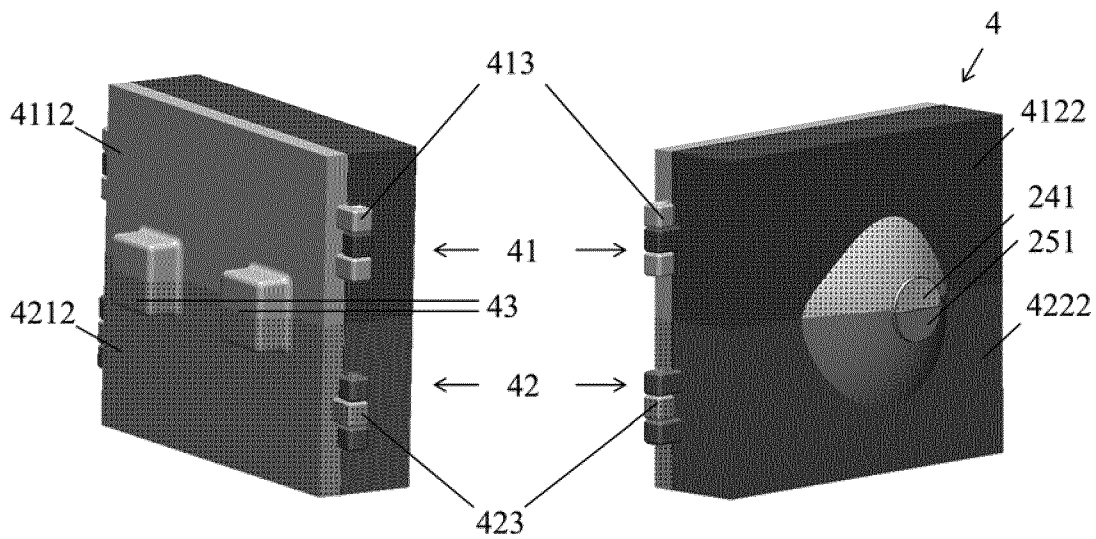


FIG. 8A

FIG. 8B

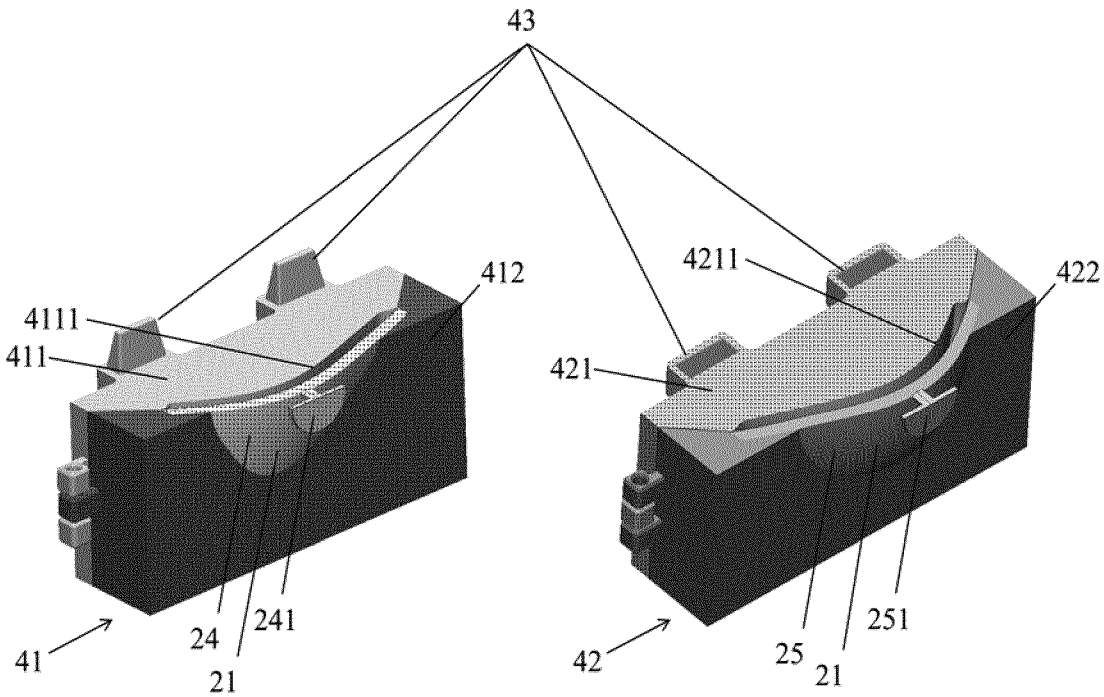


FIG. 9A

FIG. 9B

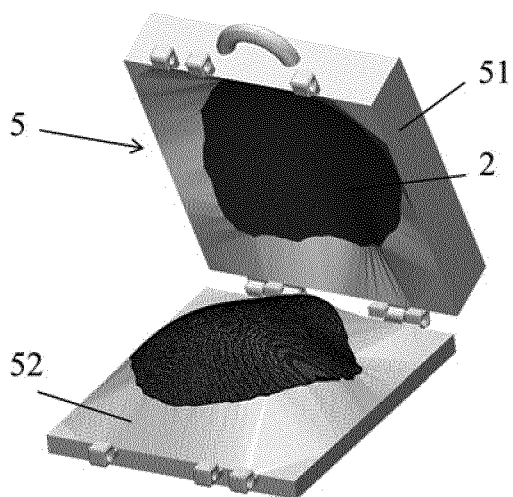


FIG. 10A

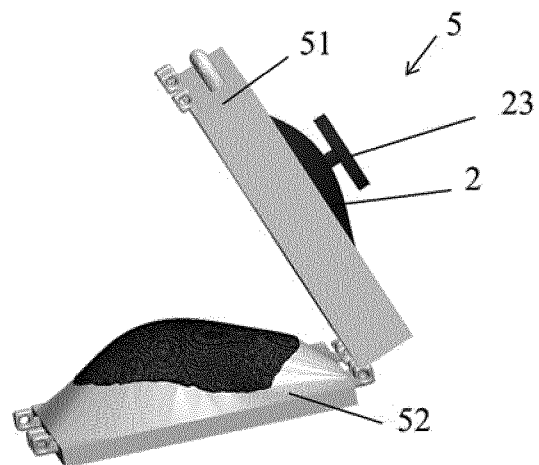


FIG. 10B

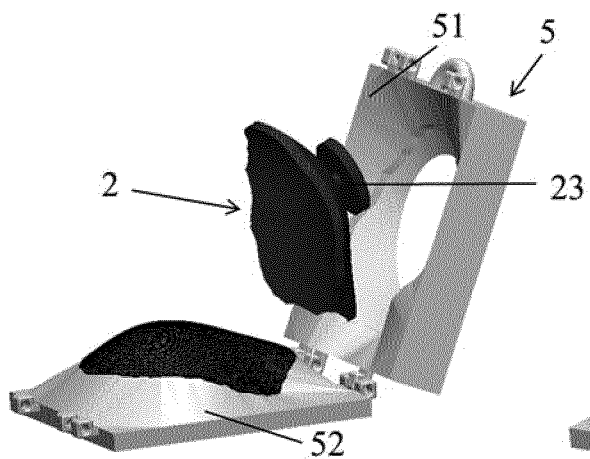


FIG. 10C

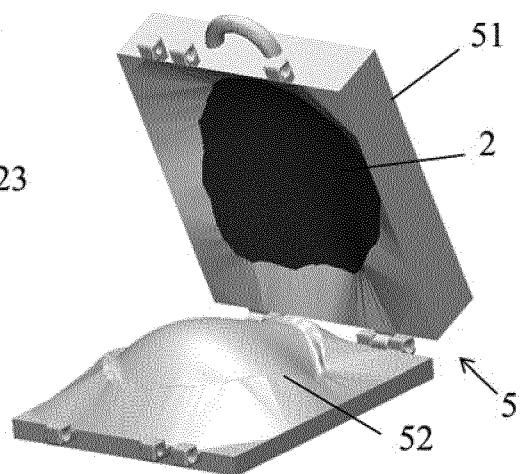


FIG. 10D

INTERNATIONAL SEARCH REPORT

International application No

PCT/EP2016/071927

A. CLASSIFICATION OF SUBJECT MATTER

INV. A61F2/28 A61F2/30 B29C33/62 B29C33/68
ADD.

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61F B29C

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EPO-Internal, WPI Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 2010/155975 A1 (HEINRICH AXEL [DE] ET AL) 24 June 2010 (2010-06-24)	1-6,8,9, 11-14
Y	paragraphs [0058] - [0060], [0105]	2,7, 10-12,15
X	WO 2012/158618 A1 (BIOMET MFG CORP [US]; SMITH DANIEL B [US]; VENDRELY TIMOTHY G [US]; KR) 22 November 2012 (2012-11-22)	1,3,4, 14,15
Y	GB 2 068 819 A (EXXON RESEARCH ENGINEERING CO) 19 August 1981 (1981-08-19)	2,7
Y	EP 1 059 153 A2 (MERCK PATENT GMBH [DE]) 13 December 2000 (2000-12-13)	10-12
	paragraphs [0009] - [0024]	
	-/--	



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

30 November 2016

Date of mailing of the international search report

09/12/2016

Name and mailing address of the ISA/

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040,
Fax: (+31-70) 340-3016

Authorized officer

Buchmann, Gerhard

INTERNATIONAL SEARCH REPORT

International application No
PCT/EP2016/071927

C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 5 397 361 A (CLARK DENNIS E [US]) 14 March 1995 (1995-03-14) column 4, lines 1-60 -----	15

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/EP2016/071927

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2010155975 A1	24-06-2010	EP 2373479 A1 US 2010155975 A1 WO 2010069961 A1	12-10-2011 24-06-2010 24-06-2010
WO 2012158618 A1	22-11-2012	AU 2012255975 A1 CA 2835030 A1 CN 103619283 A EP 2709565 A1 EP 2781205 A1 JP 2014524757 A US 2015343684 A1 WO 2012158618 A1	21-11-2013 22-11-2012 05-03-2014 26-03-2014 24-09-2014 25-09-2014 03-12-2015 22-11-2012
GB 2068819 A	19-08-1981	NONE	
EP 1059153 A2	13-12-2000	EP 1059153 A2 JP 2001058309 A	13-12-2000 06-03-2001
US 5397361 A	14-03-1995	NONE	